

AD 0648981

AFFDL-TR-66-179

DESIGN AND CONSTRUCTION OF A CRYOGENIC LIQUID LEVEL-TEMPERATURE TRANSDUCER

WILLIAM E. ALEXANDER

TECHNICAL REPORT AFFDL-TR-66-179

OCTOBER 1966

Distribution of this document
is unlimited

AIR FORCE FLIGHT DYNAMICS LABORATORY
RESEARCH AND TECHNOLOGY DIVISION
AIR FORCE SYSTEMS COMMAND
WRIGHT-PATTERSON AIR FORCE BASE, OHIO

20080819 223

NOTICES

When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

Copies of this report should not be returned to the Research and Technology Division unless return is required by security considerations, contractual obligations, or notice on a specific document.

DESIGN AND CONSTRUCTION OF A CRYOGENIC LIQUID LEVEL-TEMPERATURE TRANSDUCER

WILLIAM E. ALEXANDER

AD648981

Distribution of this document
is unlimited

FOREWORD


This report was prepared by the Experimental Mechanics Branch, Structures Division, Air Force Flight Dynamics Laboratory, Research and Technology Division, Wright-Patterson Air Force Base, Ohio.

The work reported was accomplished under Project No. 1347, "Structural Testing of Flight Vehicles," Task No. 134702, "Measurement of Structural Response." William E. Alexander was the principal investigator, while James L. Mullineaux is the task engineer.

The action was undertaken to provide pump starvation warning devices: the pumps are integral to the Structures Test Laboratory cryogenic fuel simulant system. In operation, the pipelines connected to pumps should remain full of liquid. Therefore, liquid level transducers have been installed within the pipes to give warning of pipeline evacuation. These same transducers also monitor the temperature of vaporous nitrogen at various times. These liquid level-temperature transducers were developed in the Structures Division's laboratories.

Important contributions were made by personnel of the Structures Test Branch of the Structures Division. Bernard Boggs proposed the design concept; John Taylor devised novel fabrication techniques; and Airman John Kelly conducted the performance tests.

This technical report has been reviewed and is approved.


JAMES C. HORSLEY, JR., Major, USAF
Chief, Experimental Mechanics Branch
Structures Division

ABSTRACT

This report summarizes the design and construction of a cryogenic liquid level-temperature transducer. Its sensitive element is a flattened Chromel-Alumel thermocouple. The element is heated radiantly, producing an above ambient temperature output signal. The output increases 6.5 millivolts when a drop in liquid level occurs. Ambient temperatures are monitored when the thermocouple is not heated.

TABLE OF CONTENTS

SECTION	PAGE
I INTRODUCTION	1
II PRINCIPLES OF OPERATION OF A CRYOGENIC LIQUID LEVEL TRANSDUCER	2
III DESIGN AND CONSTRUCTION	2
IV PERFORMANCE SUMMARY	3
V CONCLUSIONS	4
VI BIBLIOGRAPHY	4

ILLUSTRATIONS

FIGURE	PAGE
1. Cryogenic Liquid Level Transducer Thermal Behavior	5
2. Assembled Transducers	6
3. Cryogenic Liquid Level-Temperature Transducer Design	7
4. Thermocouple is Welded to Foil Disk	8
5. Foil Disk is Welded to Stainless Steel Tube	9
6. Electrical Circuit	10

SECTION I

INTRODUCTION

Cryogenic liquid level changes can be detected by various methods:

- a. Position changes of floating objects
- b. Gas pressure changes within tubes
- c. Spontaneous oscillation of gas in open tubes
- d. Absorption changes in gamma radiation, visible light, and thermal energy
- e. Dielectric changes

Thermal energy absorption or thermal interaction is one of the more economical methods. Functionally, several measurable parameters of a warmer object change when the object is immersed in a cryogenic liquid. The resistance, temperature, length, thermal conductivity, and other properties increase or decrease. Of these, temperature and resistance changes are easily monitored because the necessary detection devices are technically simple.

Heated resistors and thermocouples are examples of devices which react to temperature changes associated with thermal interactions. The resistor undergoes an increasing resistance as cryogenic liquid engulfing it recedes below its in situ position. The resistor, a wheat-stone bridge arm, causes bridge unbalance, and signals a liquid level change. This method would be more economical if signaling could be achieved without dependence on the wheat-stone bridge.

A heated thermocouple is more advantageous than a resistor. Its output is a direct function of thermal action at the measuring junction. No complex signal conditioning equipment is required to render the output intelligible. A thermocouple transducer would be capable of cryogenic liquid-level detection and temperature measurement. The transducer would signal liquid-level changes when the thermocouple is being heated. When no heat is applied, the output would be a function of cryogenic fluid temperature. The subject of this report is the development of such a transducer.

SECTION II

PRINCIPLES OF OPERATION OF A CRYOGENIC LIQUID LEVEL TRANSDUCER

The basic operation is outlined in Figure 1. A metal foil to which a thermocouple is attached is shown in contact with the liquid nitrogen. Radiant energy is being absorbed by both from a small resistance heater. The thermocouple signal increases sharply as the liquid surface recedes below the foil. The signal decreases to the original value when the liquid rises and contacts the foil. This signal change is proportional to the change in heat transfer rate between the foil and nitrogen. Heat is transferred by convection when the foil is within the gaseous nitrogen. However, the heat transfer is due to surface boiling upon the foil through liquid contact, and is much greater.

SECTION III

DESIGN AND CONSTRUCTION

The transducer's outer configuration is probe shaped. Two probes are shown in Figure 2, one of which has a threaded fitting.

The inner components are sketched in Figure 3, which shows that the stainless steel jacket encloses the thermocouple and heater to protect them from moving liquid forces. The protective enclosure is sealed with an Inconel foil. These components and the others were formed and assembled as follows:

- a. Seven turns of 30-gauge platinum wire around a spindle formed the miniature heater.
- b. The heater leads of 19-gauge copper wire were attached by peening.
- c. The sensing element was formed by flattening a 36-gauge Chromel-Alumel thermocouple to a 55-gauge thickness at the junction; it was then welded to the center of a 0.25-inch diameter by 0.0015-inch Inconel foil (Figure 4). In effect, an insulated attachment between the heater and the thermocouple was achieved. The air gap separating the two provided a good electrical insulator and a good thermal transmitting medium.
- d. 24-gauge Chromel-Alumel wires were used as extension leads of the finer wire thermocouple.
- e. A binding of high temperature tape secured the relative positions of the components during insertion into the 0.25-inch stainless steel tube. The tape insured firm positioning during sealing.

f. The tube was sealed with the Inconel disk by capacitance welding (Figure 5).

The components are shown with respect to a battery, an indicator, and a switch in Figure 6. These three items are not embodiments of the transducer, but are essential to its operation.

SECTION IV

PERFORMANCE SUMMARY

The transducer was designed to undergo a 5 mv change in less than 0.5 seconds. Zero would correspond to immersion in liquid nitrogen, and 5 mv to detection of cryogenic nitrogen vapor.

The completed transducers were tested to verify performance predictions. Each was energized and immersed into an open liquid nitrogen bath. The decrease in the room temperature output was recorded and the time over which the total change occurred. The power applied was varied for different tests.

Performance exceeded the design requirements. Changes were observed from 6.5 to 7 mv. The maximum time response observed was 0.15 seconds. To achieve this performance, 2.85 to 3.18 amps were applied to the transducer heaters.

SECTION V

CONCLUSIONS

An economical cryogenic liquid-level transducer can be constructed easily with inexpensive tools and the fabrication methods are simple. Other materials and thermal detectors may be used instead of those reported.

SECTION VI

BIBLIOGRAPHY

1. Corak, W. S., "A Transfer Device for Low Boiling Liquids," Review of Scientific Instruments, 1950, Vol 21, pp 583.
2. Maimoni, A. "Hot Wire Liquid-Level Indicator," 1956, Vol 27, pp 1024.
3. White, G. K. "Experimental Techniques in Low Temperature Physics," 1959, Oxford University Press.

△ - UNIT OF HEAT CONTAINED

▽ - UNIT OF HEAT FLOWING

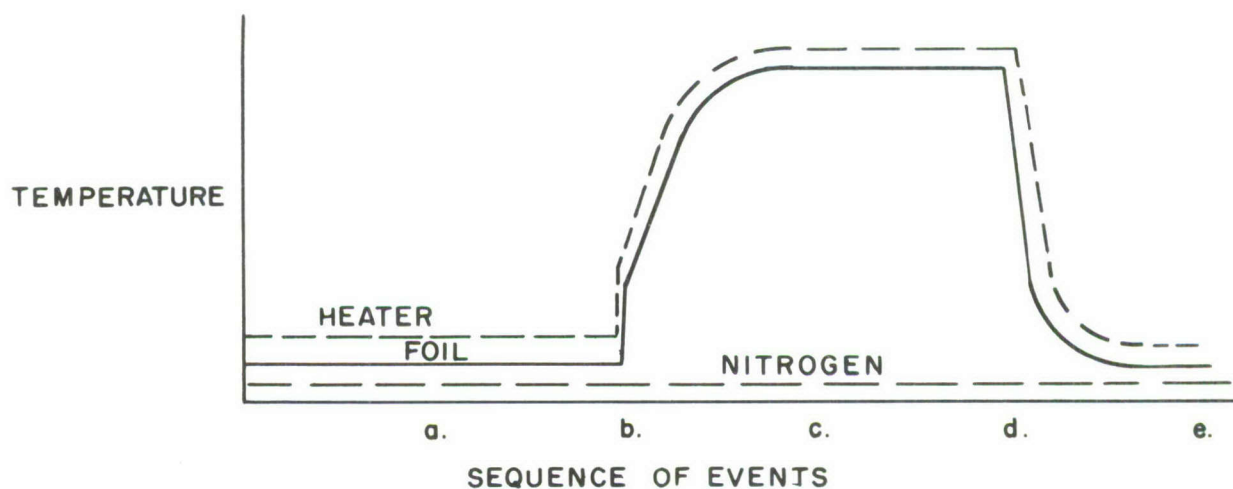
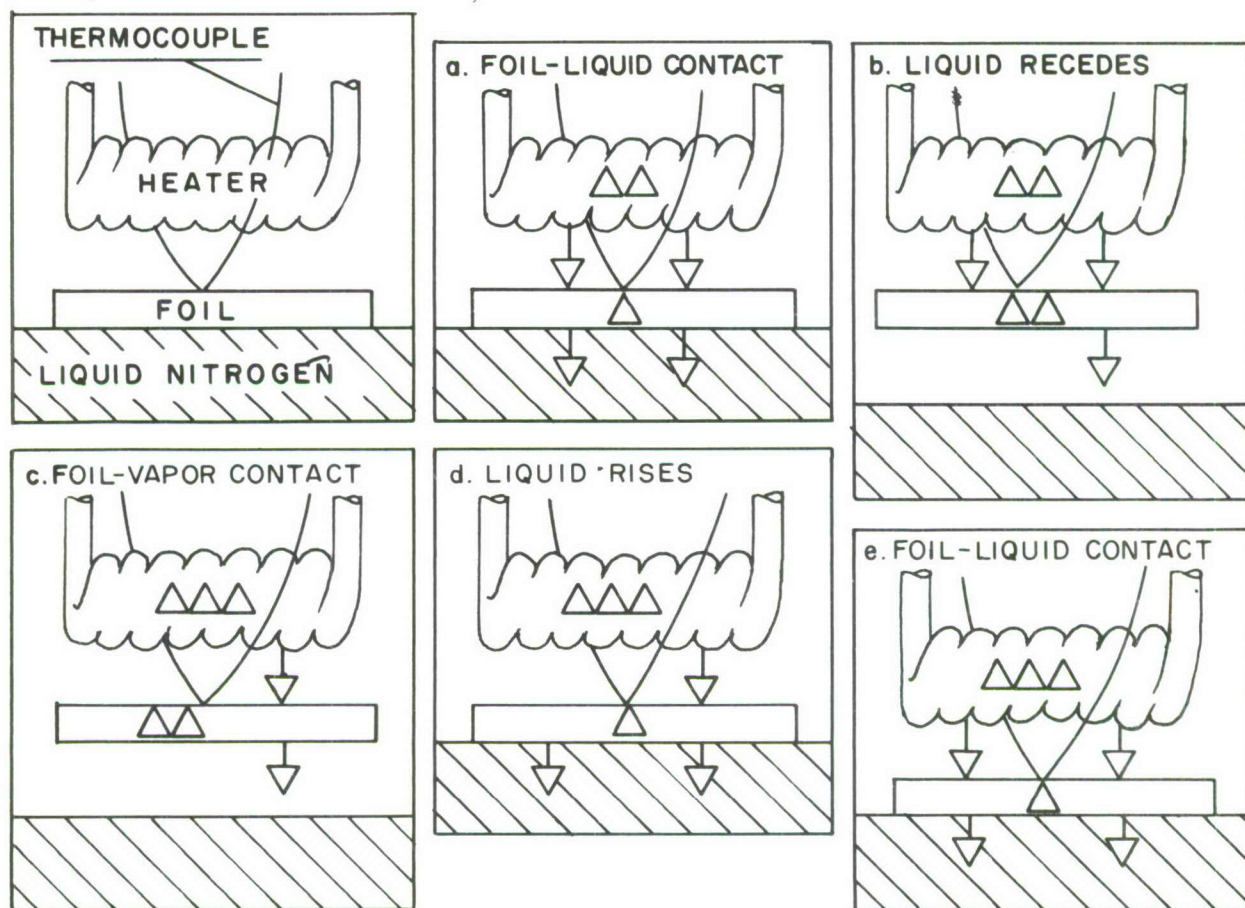


Figure 1. Cryogenic Liquid Level Transducer Thermal Behavior

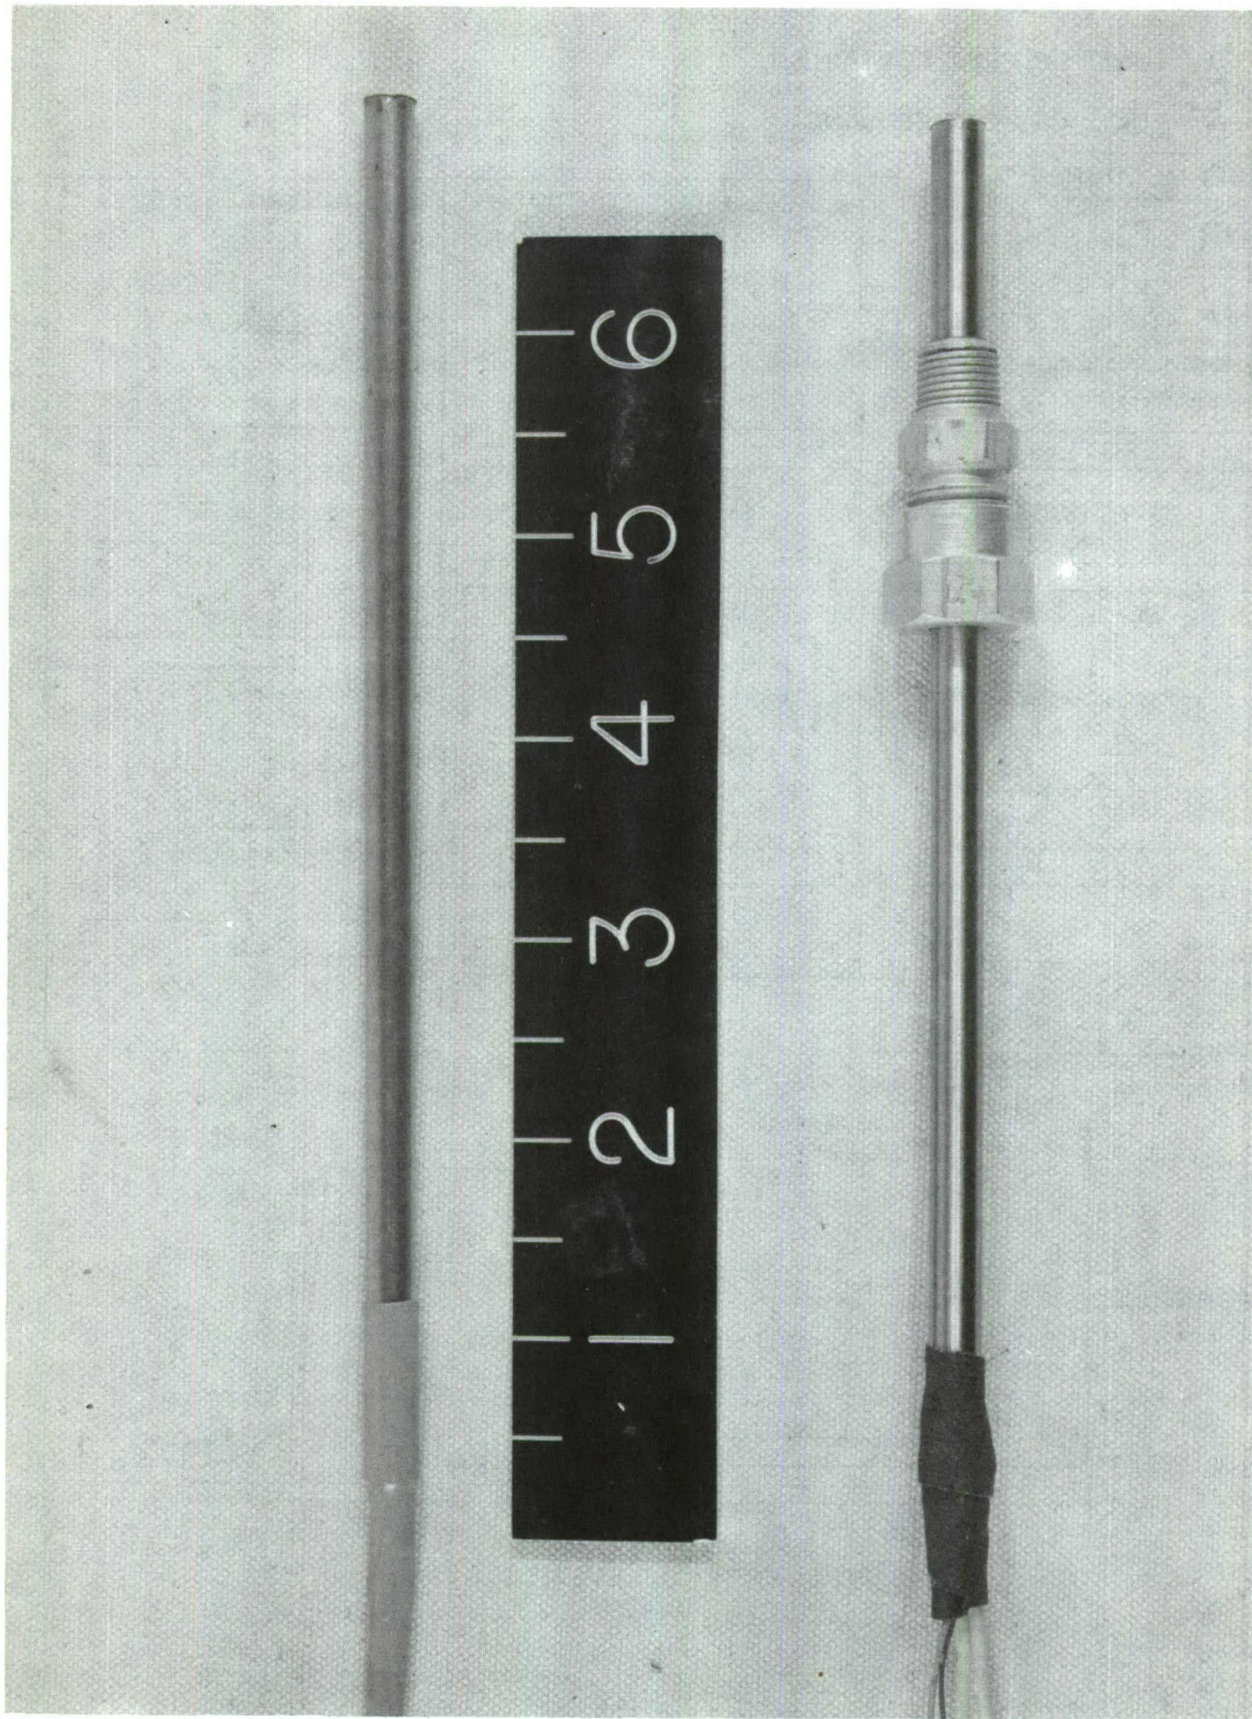


Figure 2. Assembled Transducers

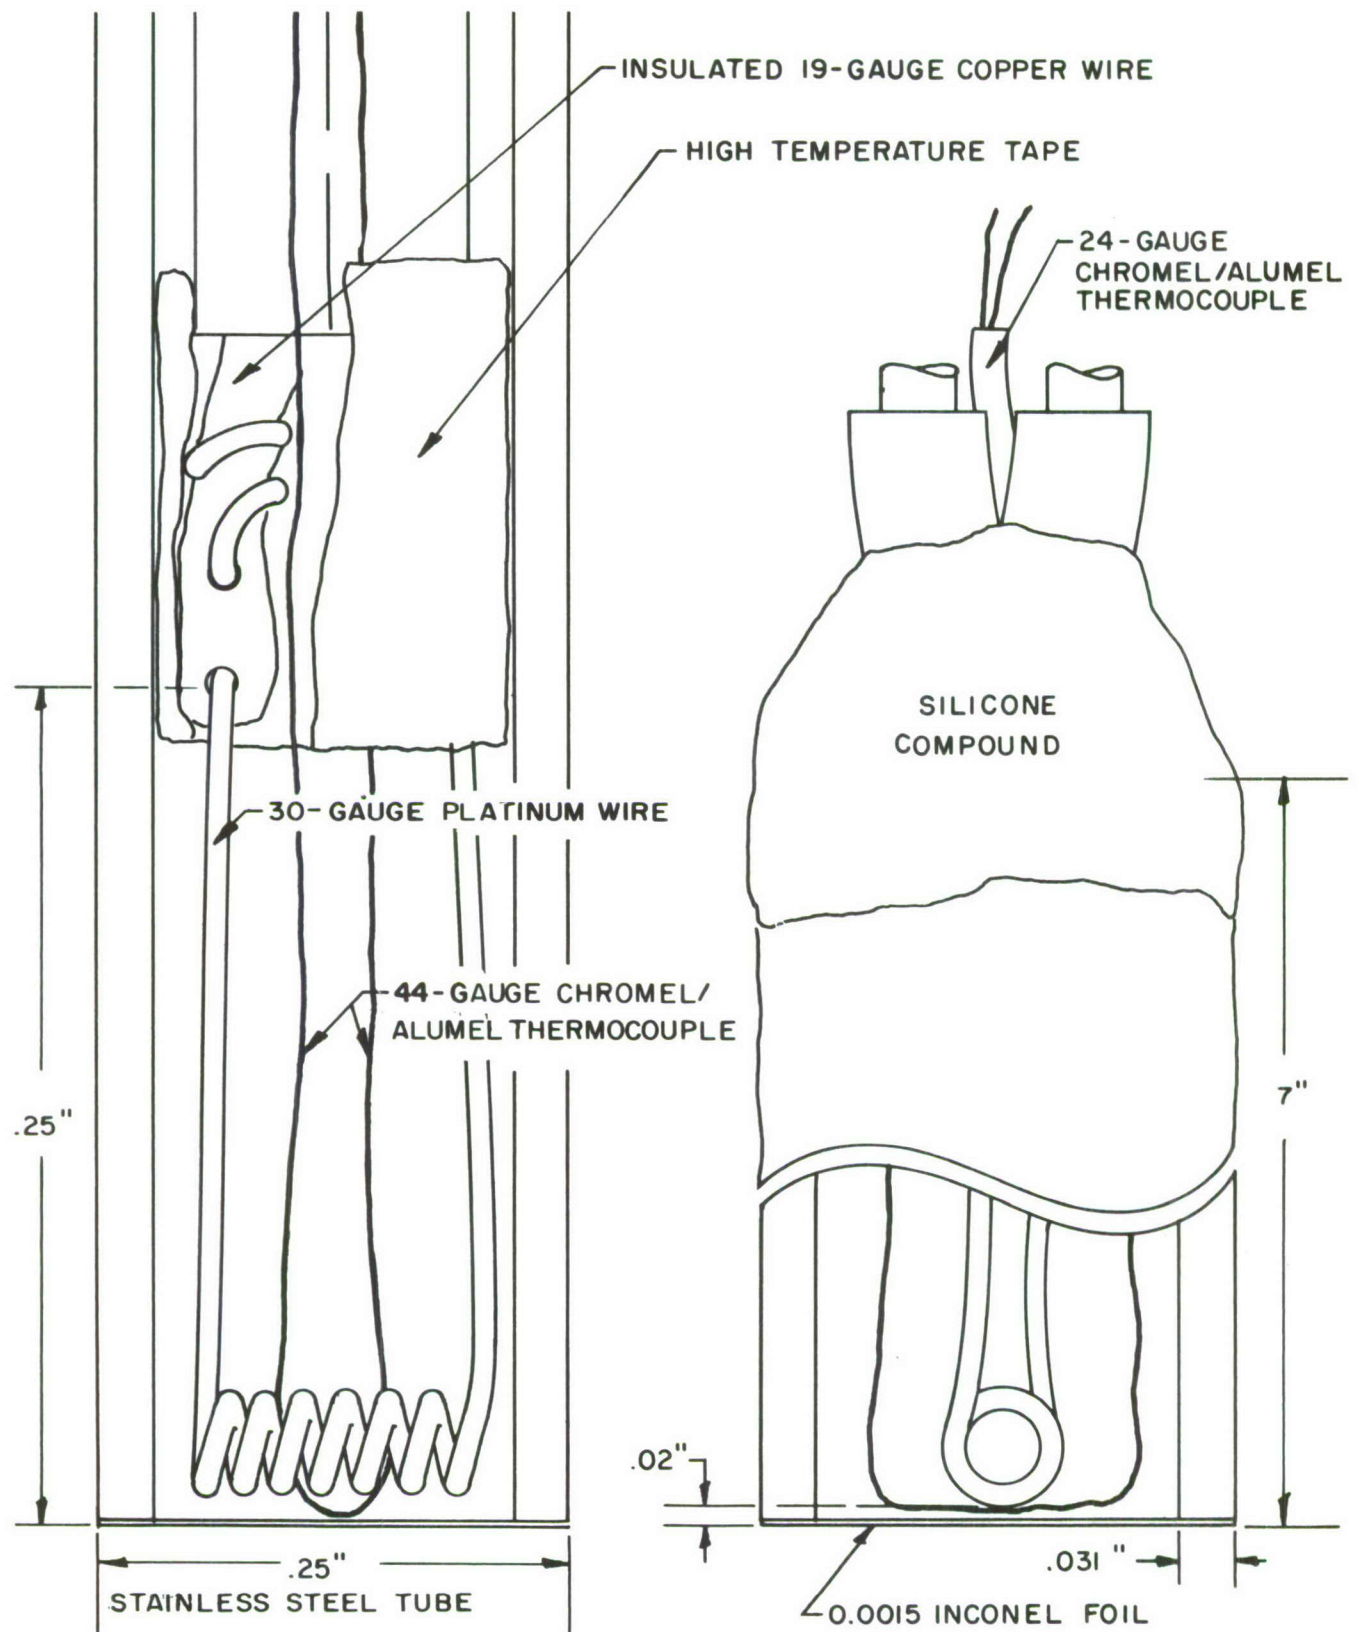


Figure 3. Cryogenic Liquid Level-Temperature Transducer Design


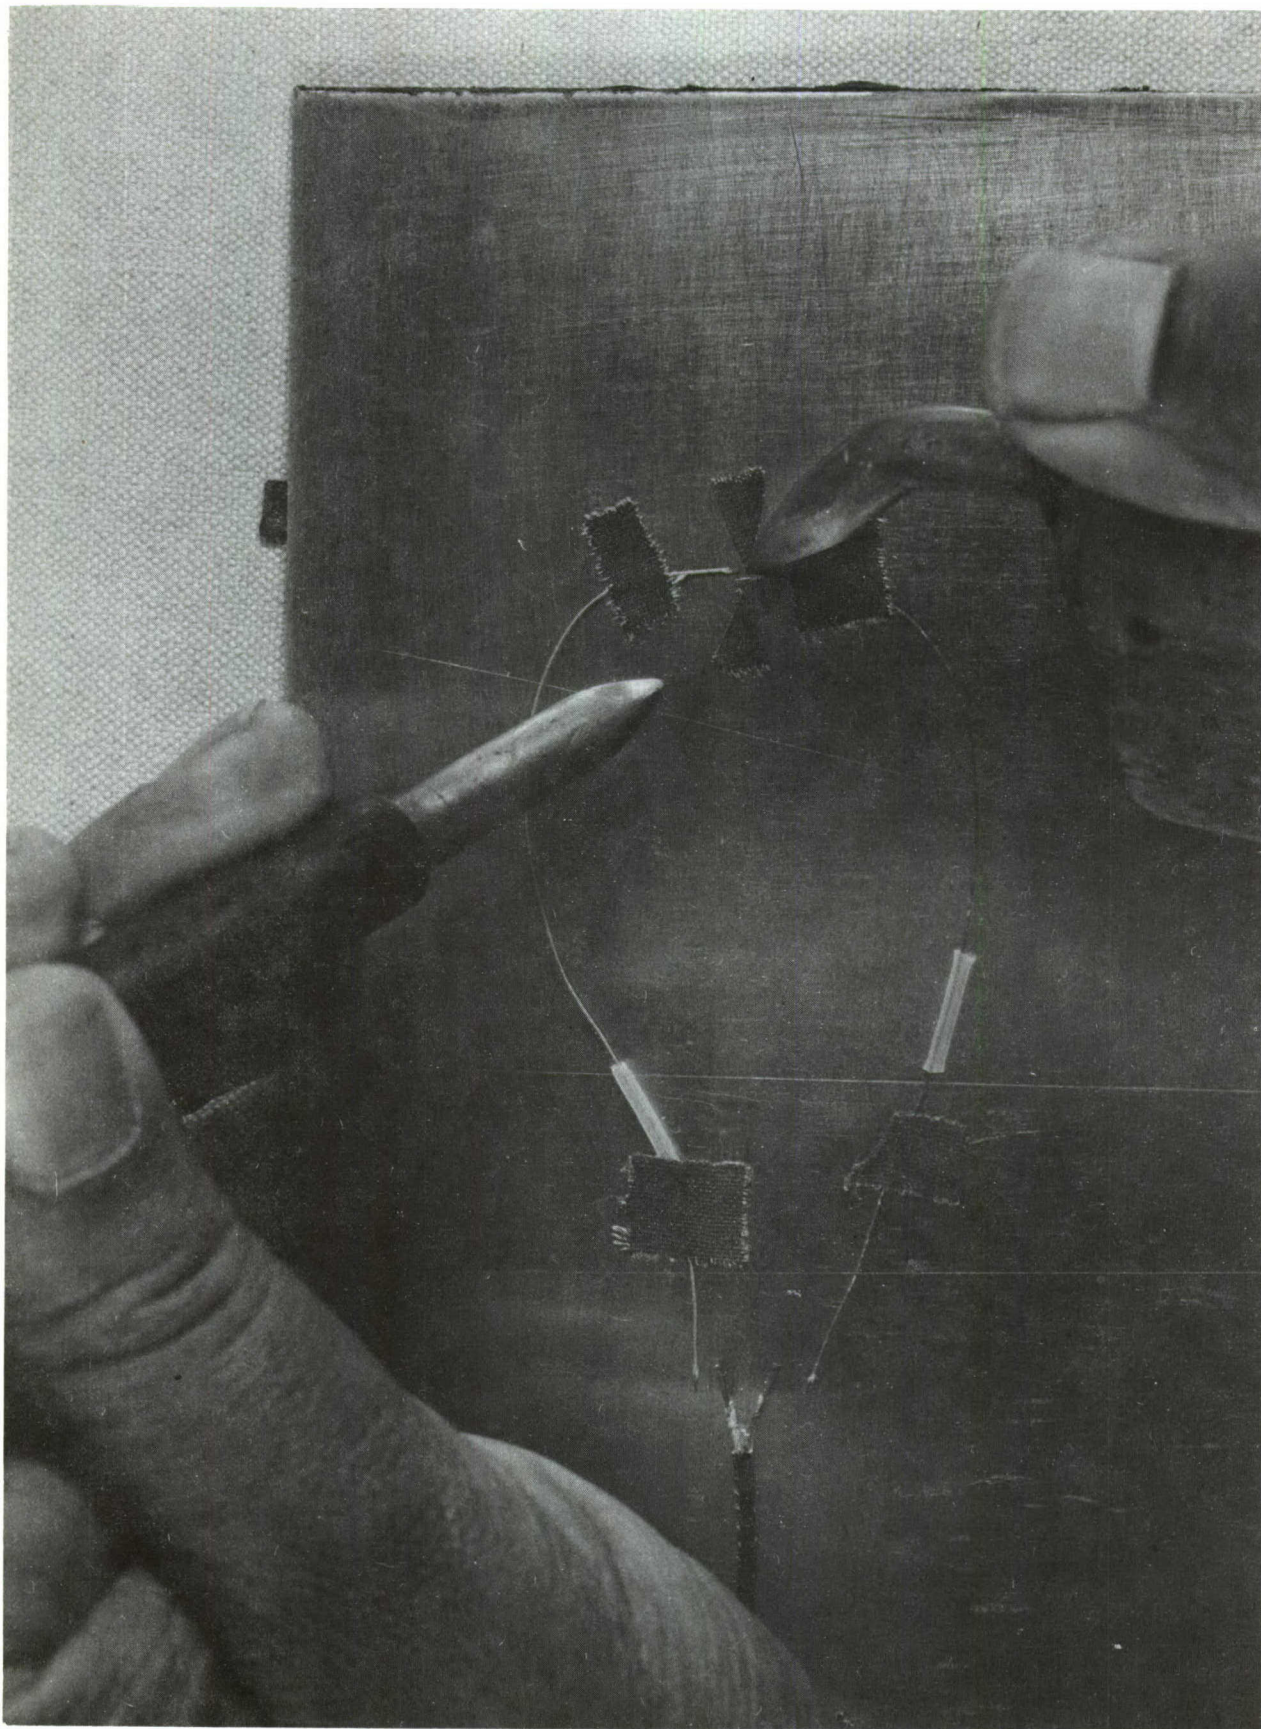


Figure 4. Thermocouple is Welded to Foil Disk



Figure 5. Foil Disk is Welded to Stainless Steel Tube

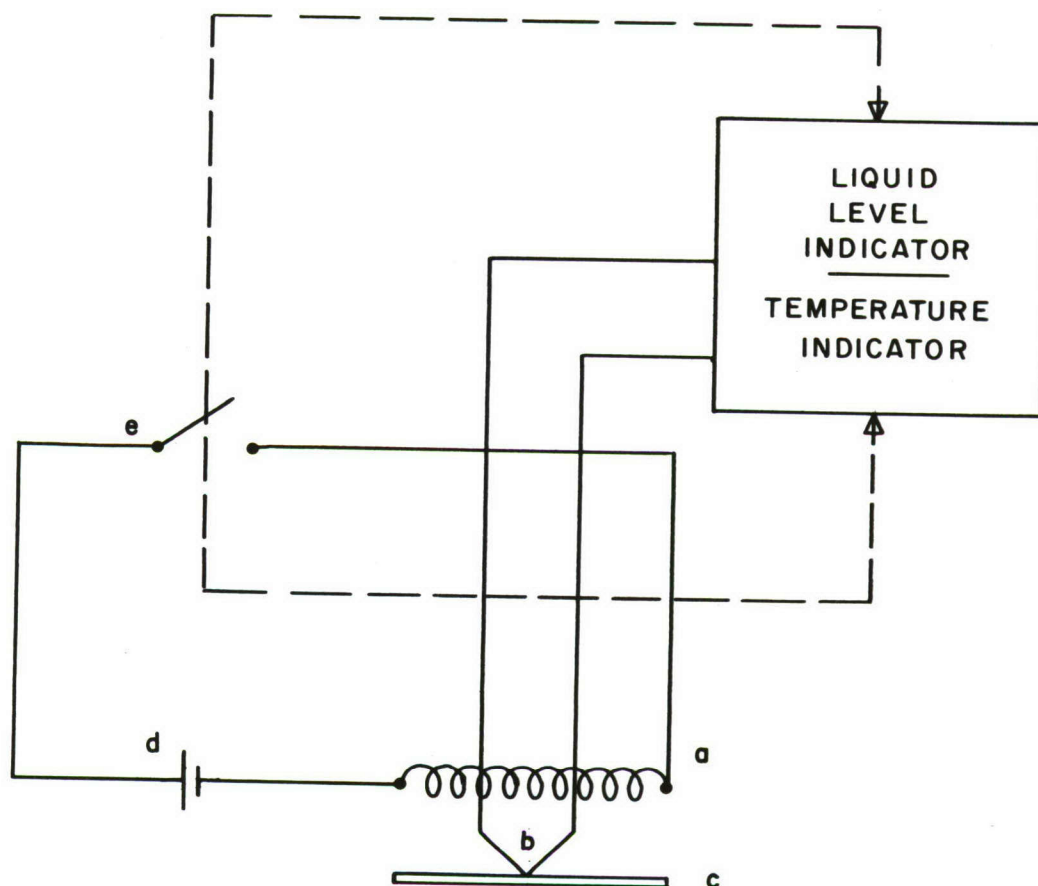

- a — HEATER
- b — THERMOCOUPLE
- c — INCONEL FOIL
- d — 1.5 VOLT BATTERY
- e — SWITCH

Figure 6. Electrical Circuit

UNCLASSIFIED

Security Classification

DOCUMENT CONTROL DATA - R&D

(Security classification of title, body of abstract and indexing annotation must be entered when the overall report is classified)

1. ORIGINATING ACTIVITY (Corporate author) Air Force Flight Dynamics Laboratory Wright-Patterson Air Force Base, Ohio		2a. REPORT SECURITY CLASSIFICATION UNCLASSIFIED	
		2b. GROUP	
3. REPORT TITLE DESIGN AND CONSTRUCTION OF A CRYOGENIC LIQUID LEVEL-TEMPERATURE TRANSDUCER			
4. DESCRIPTIVE NOTES (Type of report and inclusive dates)			
5. AUTHOR(S) (Last name, first name, initial) Alexander, William E.			
6. REPORT DATE October 1966		7a. TOTAL NO. OF PAGES 16	7b. NO. OF REFS 3
8a. CONTRACT OR GRANT NO. b. PROJECT NO. 1347 c. Task 134702 d.		9a. ORIGINATOR'S REPORT NUMBER(S) AFFDL-TR-66-179 9b. OTHER REPORT NO(S) (Any other numbers that may be assigned this report)	
10. AVAILABILITY/LIMITATION NOTICES Distribution of this document is unlimited.			
11. SUPPLEMENTARY NOTES		12. SPONSORING MILITARY ACTIVITY Air Force Flight Dynamics Laboratory Wright-Patterson Air Force Base, Ohio	
13. ABSTRACT This report summarizes the design and construction of a cryogenic liquid level-temperature transducer. Its sensitive element is a flattened Chromel-Alumel thermocouple. The element is heated radiantly producing an above ambient temperature output signal. The output increases 6.5 millivolts when a drop in liquid level occurs. Ambient temperatures are monitored when the thermocouple is not heated.			

DD FORM 1 JAN 64 1473

UNCLASSIFIED

Security Classification

14. KEY WORDS	LINK A		LINK B		LINK C	
	ROLE	WT	ROLE	WT	ROLE	WT
Liquid Level Measurement Temperature Measurement Cryogenic Measurements						

INSTRUCTIONS

1. **ORIGINATING ACTIVITY:** Enter the name and address of the contractor, subcontractor, grantee, Department of Defense activity or other organization (*corporate author*) issuing the report.

2a. **REPORT SECURITY CLASSIFICATION:** Enter the overall security classification of the report. Indicate whether "Restricted Data" is included. Marking is to be in accordance with appropriate security regulations.

2b. **GROUP:** Automatic downgrading is specified in DoD Directive 5200.10 and Armed Forces Industrial Manual. Enter the group number. Also, when applicable, show that optional markings have been used for Group 3 and Group 4 as authorized.

3. **REPORT TITLE:** Enter the complete report title in all capital letters. Titles in all cases should be unclassified. If a meaningful title cannot be selected without classification, show title classification in all capitals in parenthesis immediately following the title.

4. **DESCRIPTIVE NOTES:** If appropriate, enter the type of report, e.g., interim, progress, summary, annual, or final. Give the inclusive dates when a specific reporting period is covered.

5. **AUTHOR(S):** Enter the name(s) of author(s) as shown on or in the report. Enter last name, first name, middle initial. If military, show rank and branch of service. The name of the principal author is an absolute minimum requirement.

6. **REPORT DATE:** Enter the date of the report as day, month, year; or month, year. If more than one date appears on the report, use date of publication.

7a. **TOTAL NUMBER OF PAGES:** The total page count should follow normal pagination procedures, i.e., enter the number of pages containing information.

7b. **NUMBER OF REFERENCES:** Enter the total number of references cited in the report.

8a. **CONTRACT OR GRANT NUMBER:** If appropriate, enter the applicable number of the contract or grant under which the report was written.

8b, 8c, & 8d. **PROJECT NUMBER:** Enter the appropriate military department identification, such as project number, subproject number, system numbers, task number, etc.

9a. **ORIGINATOR'S REPORT NUMBER(S):** Enter the official report number by which the document will be identified and controlled by the originating activity. This number must be unique to this report.

9b. **OTHER REPORT NUMBER(S):** If the report has been assigned any other report numbers (*either by the originator or by the sponsor*), also enter this number(s).

10. **AVAILABILITY/LIMITATION NOTICES:** Enter any limitations on further dissemination of the report, other than those

imposed by security classification, using standard statements such as:

- (1) "Qualified requesters may obtain copies of this report from DDC."
- (2) "Foreign announcement and dissemination of this report by DDC is not authorized."
- (3) "U. S. Government agencies may obtain copies of this report directly from DDC. Other qualified DDC users shall request through _____."
- (4) "U. S. military agencies may obtain copies of this report directly from DDC. Other qualified users shall request through _____."
- (5) "All distribution of this report is controlled. Qualified DDC users shall request through _____."

If the report has been furnished to the Office of Technical Services, Department of Commerce, for sale to the public, indicate this fact and enter the price, if known.

11. **SUPPLEMENTARY NOTES:** Use for additional explanatory notes.

12. **SPONSORING MILITARY ACTIVITY:** Enter the name of the departmental project office or laboratory sponsoring (*paying for*) the research and development. Include address.

13. **ABSTRACT:** Enter an abstract giving a brief and factual summary of the document indicative of the report, even though it may also appear elsewhere in the body of the technical report. If additional space is required, a continuation sheet shall be attached.

It is highly desirable that the abstract of classified reports be unclassified. Each paragraph of the abstract shall end with an indication of the military security classification of the information in the paragraph, represented as (TS), (S), (C), or (U).

There is no limitation on the length of the abstract. However, the suggested length is from 150 to 225 words.

14. **KEY WORDS:** Key words are technically meaningful terms or short phrases that characterize a report and may be used as index entries for cataloging the report. Key words must be selected so that no security classification is required. Identifiers, such as equipment model designation, trade name, military project code name, geographic location, may be used as key words but will be followed by an indication of technical context. The assignment of links, rules, and weights is optional.